Volume 26 Numbers 1–6 January–December 2002

Journal of Medical Engineering & Technology

An international bimonthly journal promoting the application of engineering and technology in medical research and clinical medicine

Editor in Chief

Emeritus Professor M. M. Black
University of Sheffield
c/o 26 Broad Elms Lane
Sheffield S11 9RQ

North American Editor

Dr M.J. Thubrikar
(Associate Director)
Heineman Medical Research Laboratories
Carolinas Medical Center
1000 Blythe Blvd.
Charlotte, NC 28203, USA

Adjunct Professor of Biomedical Engineering
University of North Carolina, Charlotte, NC, USA

Associate Editors

Dr D. C. Crawford
(Evaluation & MDA News)
CEDAR (Clinical Engineering
Device Assessment and Reporting)
Cardiff Medicentre
Heath Park
Cardiff CF14 4UJ

Dr J. Fenner
(News & Product Update)
Department of Medical Physics
& Clinical Engineering
University of Sheffield
Royal Hallamshire Hospital
Glossop Road
Sheffield S10 2JF

Dr P. V. Lawford
(Selected Contents & Book Reviews)
Department of Medical Physics
& Clinical Engineering
University of Sheffield
Royal Hallamshire Hospital
Glossop Road
Sheffield S10 2JF

Editorial Committee

Professor J. Edwards
Highbank,
Ravenhurst Drive
Bolton BL1 5DL

Dr S. Meldrum
Department of Medical
Physics & Bioengineering
Norfolk & Norwich Hospital
Norwich NR1 3SR

Dr S. W. Smye
Medical Physics Department
St James's University Hospital
Beckett Street
Leeds LS9 7TF

Professor I. A. Sutherland
Brunel Institute for Bioengineering
Brunel University
Uxbridge
Middlesex UB8 3PH

Dr D. Tayler
225 Ringing Low Road
Sheffield S11 7PT

Dr W. Wain
Sorin Biomedica
Holmbush Estate
Midhurst
West Sussex GU29 9HX

Professor J. P. Woodcock
Department of Medical
Physics & Bioengineering
University Hospital of Wales
Heath Park, Cardiff CF4 4XW

Taylor & Francis
healthsciences

Contents of Volume 26 (2002)

NUMBER 1 JANUARY–FEBRUARY 2002

The time relationships of the constituent components of the human electrocardiogram
M.J. Burke and M. Nasor 1

QRS detection using new wavelets
S.C. Saxena, V. Kumar and S.T. Hamde 7

Preliminary study of potential for rapid prototype and surface scanned radiotherapy facemask production technique
B. Sanghera, A. Amis and M. McGurk 16

Electrical current distribution under transthoracic defibrillation and pacing electrodes
S. Papazov, Z. Kostov and I. Daskalov 22

Force assessment of the stimulated arm flexors: quantification of contractile properties
J.B. Hong and P.A. Iaizzo 28

Permanent magnetic-levitation of rotating impeller: a decisive breakthrough in the centrifugal pump
K.X. Qian, P. Zeng, W.M. Ru, H.Y. Yuan, Z.G. Feng and L. Li 36

Differences in foetal heart rate variability from phonocardiography and abdominal electrocardiography
R. Ortiz, R. González, M.A. Peña, S. Carrasco, M.J. Gaitán and C. Vargas 39

MDA Publications 46

News & Product Update 49

Calendar 52

Addendum 53

NUMBER 2 MARCH–APRIL 2002

Hardware design for the computation of heart rate variability
A. Alexandridi and G. Manis 49

Energetic parameter changes with mechanical ventilation in conjunction with BVAD assistance
C. De Lazzari, M. Darowski, G. Ferrari, F. Clemente and M. Guaragno 63

Neonatal life support during magnetic resonance imaging
F. Groenendaal, C. Leusink, M. Nijenhuis and M.J.H. Janssen 71

Abdominal aortic aneurysm and stent graft phantom manufactured by medical rapid prototyping
R.J. Winder, Z. Sun, B. Kelly, P.K. Ellis and D. Hirst 75

Streamlined design of impeller and its effect on pump haemolysis
K.X. Qian, P. Zeng, W.M. Ru and H.Y. Yuan 79

Humidity control of an incubator using the microcontroller-based active humidifier system employing an ultrasonic nebulizer
I. Güler and M. Burunkaya 82

MDA Publications 89

News & Product Update 91

Calendar 94

NUMBER 3 MAY–JUNE 2002

New tridimensional approach to the evaluation of the spine through surface measurement: the BACES system
F. D'Osualdo, S. Schierano, F.M. Soldano and M. Isola 95

Paraplegics standing up using multichannel FES and arm support
J. Kuželički, R. Kamnik, T. Bajd, P. Obreza and H. Benko 106

Analysis of the operation of the SCD Response intermittent compression system
Rh.J. Morris, H. Griffiths and J.P. Woodcock 111

Digital envelope detector for blood pressure measurement using an oscillometric method
J.Y. Lee, J.K. Kim and G. Yoon 117

Development of a continuous temperature mapping system using a deep body thermometer
T. Matsui, K. Hagisawa, T. Ishizuka, K. Matsumura, M. Ishihara, S. Sato, B. Takase, M. Suzuki, M. Kikuchi and A. Kurita 123

Instrument for scanning the angular variation of irradiance in ultraviolet phototherapy cabinets
A.L. Evans, C.J. Martin, D.C. Smith, G.D. Currie, S. McCalman, D. Bilsland and S. Dunn 126

MDA Publications 132

News & Product Update 134

Calendar 137

NUMBER 4 JULY–AUGUST 2002

Intelligent multifunction myoelectric control of hand prostheses
C.M. Light, P.H. Chappell, B. Hudgins and K. Englehart 139

An instrument to investigate temporal processing mechanisms with the multifocal ERG
D.C. Smith, D. Keating, S. Parks and A.L. Evans 147

Computerized detection of breast cancer with artificial intelligence and thermograms
E.Y.-K. Ng, S.C. Fok, Y.C. Peh, F.C. Ng and L.S.J. Sim 152

Continuous amperometric monitoring of subcutaneous oxygen in rabbit by telemetry
W.K. Ward, M.D. Wood and E.P. Slobodzian 158

Electric current perception study challenges electric safety limits
N. Leitgeb and J. Schroettner 168

Technical Note: SEMG-controlled telephone interface for people with disabilities
Y.-L. Chen, J.-S. Lai, J.-J. Luh and T.-S. Kuo 173

MDA Publications 177

News & Product Update 180

Calendar 184

NUMBER 5 SEPTEMBER–OCTOBER 2002

The credibility of the breast cancer risk assessment (BCRA) tool for Asians
E.Y.-K. Ng, Y.H. Chiok and S.H. Heng 185

On modelling the kinestatic charge detector for digital radiographic diagnostic and portal imaging
G. Qi, M.Y. Goloubev, F.A. DiBianca and S. Samant 193

Technical note: Experimental method to reveal the effect of rotor magnet size and air gap on artificial heart driving motor torque and efficiency
K.X. Qian, H.Y. Yuan, W.M. Ru and P. Zeng 199

Morse code recognition system with fuzzy algorithm for disabled persons
C.-M. Wu and C.-H. Luo 202

An accurate amperometric glucose sensor based glucometer with eliminated cross-sensitivity
M.M. Bani Amer 208

Technical note: A novel impeller TAH using magnetic bearings for load reduction
K.X. Qian, W.M. Ru, P. Zeng and H.Y. Yuan 214

Motorized head impulse stimulator to determine angular horizontal vestibulo-ocular reflex
H. Aalto, T. Hirvonen and M. Juhola 217

A methodological approach for the characterization of cardiac pacemaker immunity to low frequency interferences: case of 50 Hz, 60 Hz, 10 kHz and 25 kHz led disruptions
A. Hedjiedj, C. Goeury and M. Nadi 223

MDA Publications 228

Calendar 230

NUMBER 6 NOVEMBER–DECEMBER 2002

Global bioheat model for quick evaluation of the human physiological thermal profiles under differing conditions
Y.H. Chiok, E.Y.-K. Ng and V.V. Kulish 231

Quantitative evaluation of the dynamics of external factors influencing canine gastric electrical activity before and after uncoupling
C.N. Price and M.P. Mintchev 239

Logarithmic amplifier for computed tomography tasks using fluoroscopic projections
I. Buliev, C. Badea and N. Pallikarakis 247

Comparison between the analgesic and therapeutic effects of a musically modulated electromagnetic field (TAMMEF) and those of a 100 Hz electromagnetic field: blind experiment on patients suffering from cervicla spondylosis or shoulder periarthritis
M. Rigato, E. Battisti, M. Fortunato and N. Giordano 253

Early online detection of upper airway obstructions in obstructive sleep apnoea syndrome (OSAS) patients
M. Kermit, A.J. Eide and T. Lindblad 259

A new impact actuator using linear momentum exchange of inertia mass
H.-J. Min, H.-J. Lim and S.H. Kim 265

MDA Publications 270
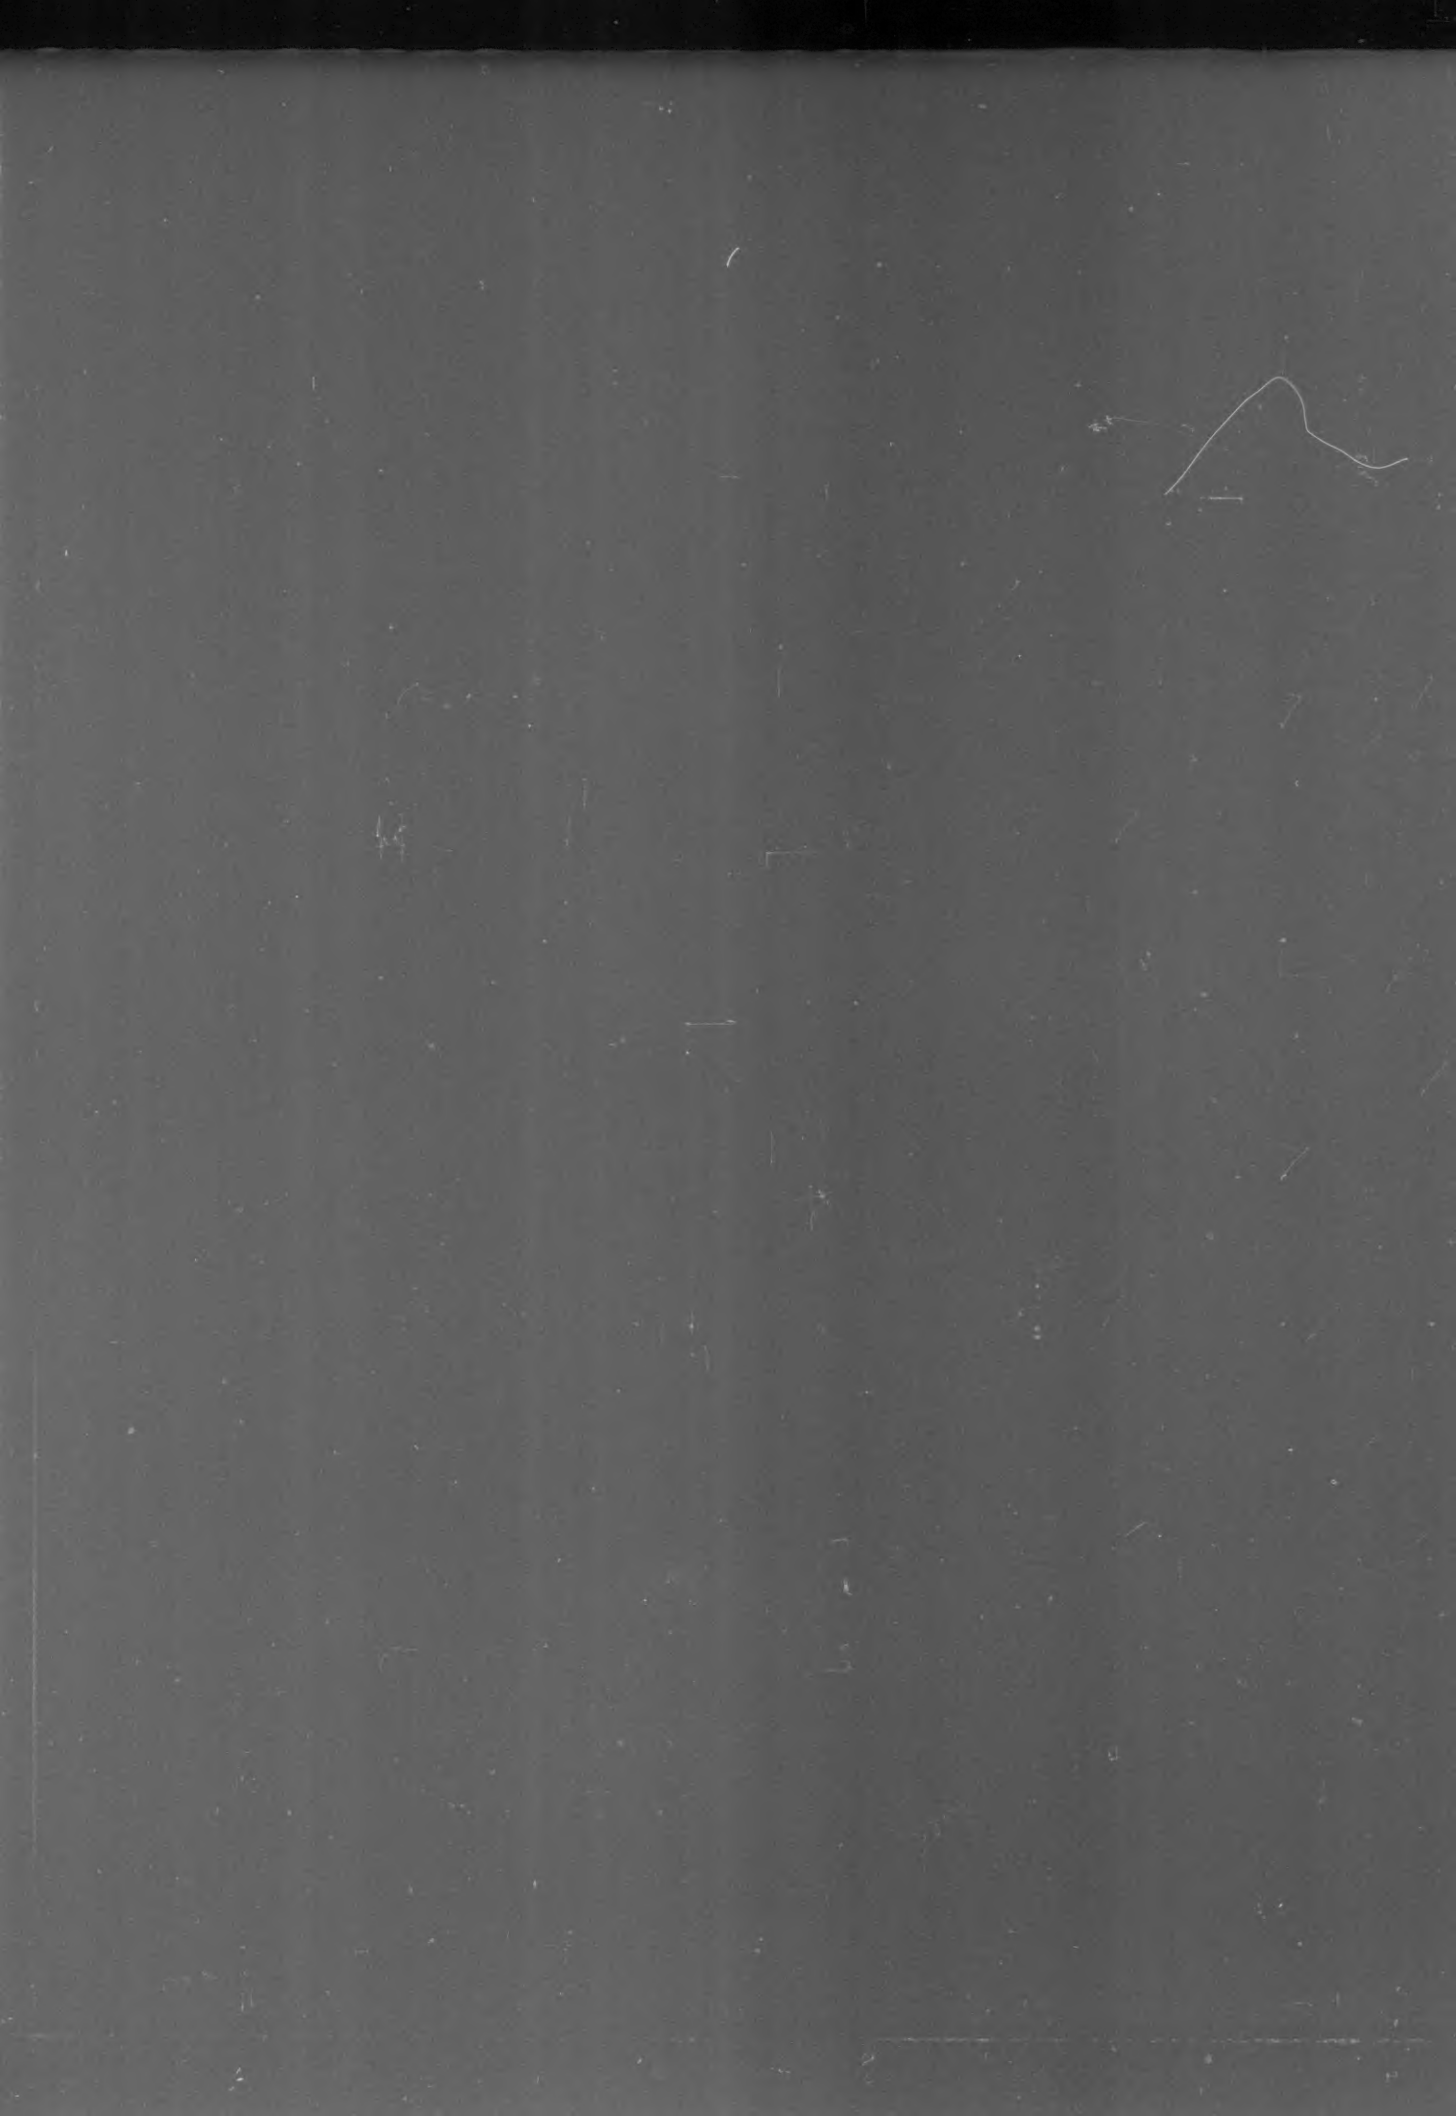
Calendar 273